

Inside the November Issue

MON TASTIC

# HEALTHCARE PURCHASING NEWS



Follow @HPN\_Online

CLINICAL INTELLIGENCE FOR SUPPLY CHAIN LEADERSHIP

Like us on Facebook



Transitioning from "Value of Products" to "Value of Care" with Analytics



Click the cover above for the online edition, or click below for the digital flip book.

## INSIDE THE CURRENT ISSUE

November 2014

### 2014 Endoscope Care Guide



#### When are endoscopes, heat-sensitive devices ready to be handled safely?

by Kaumudi Kulkarni, M.S.

In sterile processing, knowing if the endoscopes and other heat sensitive devices are ready to be safely handled is of the utmost importance. The wide array of medical devices can be grouped under three rubrics based on how they are cleaned: Manually cleaned, machine-cleaned or a combination of both.



Fig. 1 - Manually cleaned devices

A question I hear often is: Are manually cleaned devices safe to handle? Manually cleaned devices are generally perceived to be not as safe to handle, as the mechanically cleaned instruments. Many sterile processing personnel even take the added step of wiping the manually cleaned items with alcohol after they have been sent through the pass-through window. Manual cleaning is required for devices that are temperature sensitive, non-submersible or those that have size limitations (Fig. 1). Rigid endoscopes including arthroscopes and laparoscopes that have power cords, lenses and electronics components are often manually cleaned for the same reasons.

There is a novel concept that adds a level of safety to handling manually cleaned devices on the clean side of the sterile

#### NOVEMBER 2014 Featured advertisers:

- [3M Tegaderm CHG](#)
- [AHRMM](#)
- [AirClean Systems](#)
- [Baxter Healthcare Corporation](#)
- [Bioquell](#)
- [Censis Technologies](#)
- [Dale Medical Products Inc.](#)
- [Diversey Care](#)
- [Duracell Professional](#)
- [Exergen Corp.](#)
- [Halyard Health](#)
- [Healthmark Industries](#)
- [Henry Schein](#)
- [IAHCSMM](#)
- [IMS](#)
- [Karl Storz Endoscopy](#)
- [Medivators Inc.](#)
- [MHI](#)
- [Midmark](#)
- [Mighty Badge](#)
- [Mobile Instrument Service](#)
- [Olympus America](#)
- [One Source](#)
- [Palmero Health Care](#)
- [Parker Labs Inc.](#)

November Cover Story

[Celebrating a decade of device advice](#)

## HPN 2015 INDUSTRY GUIDE

[Self Study Series](#)

[White Papers](#)

[Purchasing Connection](#)

[Resources](#)

[Show Calendar](#)

[HPN Hall of Fame](#)

[HPN Buyers Guides](#)

**SHOP HPN**  
FEATURED PRODUCTS  
INFORMATION LINK

[Classifieds](#)

[Issue Archives](#)

[Advertise](#)

[About Us](#)

[Contact Us](#)

[Subscribe](#)

 **Sign up for our Email Newsletter**

Privacy by  **SafeSubscribe<sup>SM</sup>**  
For Email Marketing you can trust

**HOME**

KSR Publishing, Inc.  
Copyright © 2014

processing area. This no-touch technology does not replace manual cleaning, but supplements it. The concept is to pass the manually cleaned devices from the decontamination side to the clean side through an ultraviolet (UV) disinfection system that is placed in the pass through window (Fig. 2). This way, the manually cleaned devices are further disinfected before they come to the clean side. This concept is similar to the well-established use of UV radiation to disinfect hospital rooms.



Fig. 2 -UV Disinfector placed at Pass through window

UV light is a small part of the entire electromagnetic spectrum, which is made up of other types of radiation including gamma ray, X-rays, visible light, infrared, microwaves and radio waves, all at different wavelengths. UV disinfection has long been known and is an accepted practice in the medical field since the mid-20th century.

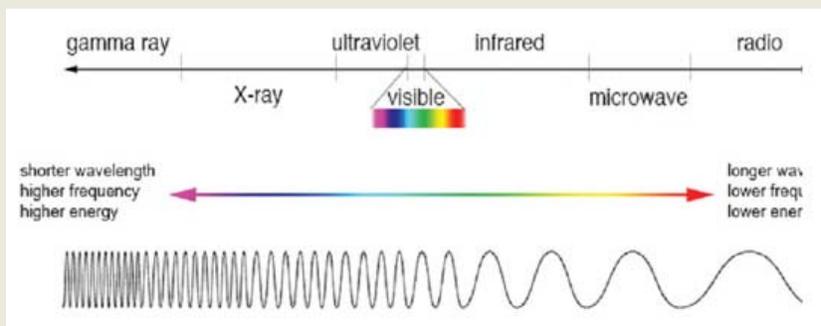


Fig. 3 - The Electromagnetic Spectrum

UV light is very versatile and can be used for disinfecting water as well as destroying harmful microorganisms on surfaces and in the air. The UV light spectrum can be broadly sub-divided into the following energy bands, distinguished by the radiation wavelengths: UV-A, UV-B, UV-C and Vacuum UV (Fig. 3). It is the intensive UV-C radiation, in the wavelength range of 254 nm that reaches the microorganisms and directly impacts their DNA. The mode of action of the UV-C radiation is that it breaks the molecular bonds inside microbial DNA, thus destroying the germ and its pathogenic effects.

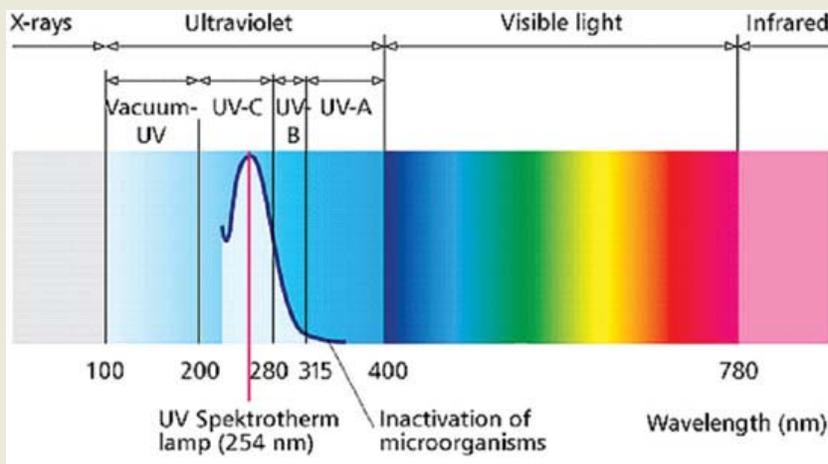


Fig. 4 - UV Light Spectrum - Image Courtesy: wedeco.com

To evaluate the use of UV

- [PDI](#)
- [Rubbermaid Commercial Products](#)
- [Ruhof Corporation](#)
- [Tronex Healthcare Industries](#)
- [Veritiv](#)
- [VHA](#)
- [World Congress](#)

disinfection at the pass through window, an independent study was conducted on cleaned instruments. In the study, 14 manually cleaned and 49 mechanically cleaned medical devices were obtained from local area hospitals. The design of the experiment was to obtain a count of bacteria growing on the medical devices from both the device sets. After swabbing, the clean devices were passed through the UV disinfectant (Fig. 5). The cycle time of the UV disinfectant was one minute. A bacterial count was taken on both the manually and mechanically cleaned instruments after they came out of the UV disinfectant.



Fig. 5 - UV Flash Disinfectant provided by Midbrook Medical, Jackson, MI

UV sensitive chemical indicators (Fig. 5) were used to help ensure that the inside chamber of the UV disinfectant was indeed exposed to the 254 nm wavelength. These indicators are specifically designed to monitor the UV radiation dosage in UV-C disinfection systems. When exposed to a UV radiation of 254nm for an extended period of time, the indicators demonstrate a distinct color shift that provides a simple visual confirmation.



Fig. 6 - UV Indicator from Healthmark Industries, Fraser, MI

The study demonstrated that the manually cleaned devices did have a higher bacterial colony-forming units (CFU) count than the machine-washed items and that the UV radiation did result in significant reduction of the CFU counts, thereby improving the safety of handling these instruments.

It is well established that with UV light technology it is possible to destroy a large number of harmful microorganisms, inexpensively and with high efficiency, without the addition of chemicals and without harmful side effects.

Hearing staff concerns and addressing their issues by bringing new research into practice is the mantra for an ever evolving sterile processing department. At the end I would like to say do your due diligence, because when it comes to safety, tomorrow is too late, today is about time!

Kaumudi Kulkarni, M.S., is Business Development Microbiologist, [Healthmark Industries](#).

## Inside...

### Sterile Processing

- [1. Endoscopic accessories strive to match visual technology advances](#)
  - [a. How has endoscope care changed in the last decade?](#)
- [2. SPD's most pressing endoscopic issues](#)
  - [a. Debunking endoscope reprocessing myths](#)
  - [3. Making sense of manufacturer reprocessing guidelines](#)
    - [a. Sterile processing head scratchers](#)
    - [b. Justifying immediate-use sterilization](#)
  - [4. When are endoscopes, heat-sensitive devices ready to be handled safely?](#)

### Maintenance & Repairs

- [6. Spotting those endoscope maintenance warning signs](#)
    - [a. Straight dope on inspecting scopes](#)
  - [7. Repair or replace? That is the question](#)
    - [a. Exploring, justifying certified pre-owned endoscopes](#)
    - [8. Third party vs. OEM for repairs?](#)
- ### Storage & Tracking
- [9. Tracking scopes - Periscopes for endoscopes](#)
    - [a. Endoscope storage techniques that work](#)
  - [10. When does outsourcing endoscope](#)

[5. Enzymatic detergent selection tips](#)

[care make sense?](#)

**Extras**

[11. Endoscope Product Spotlights](#)

