



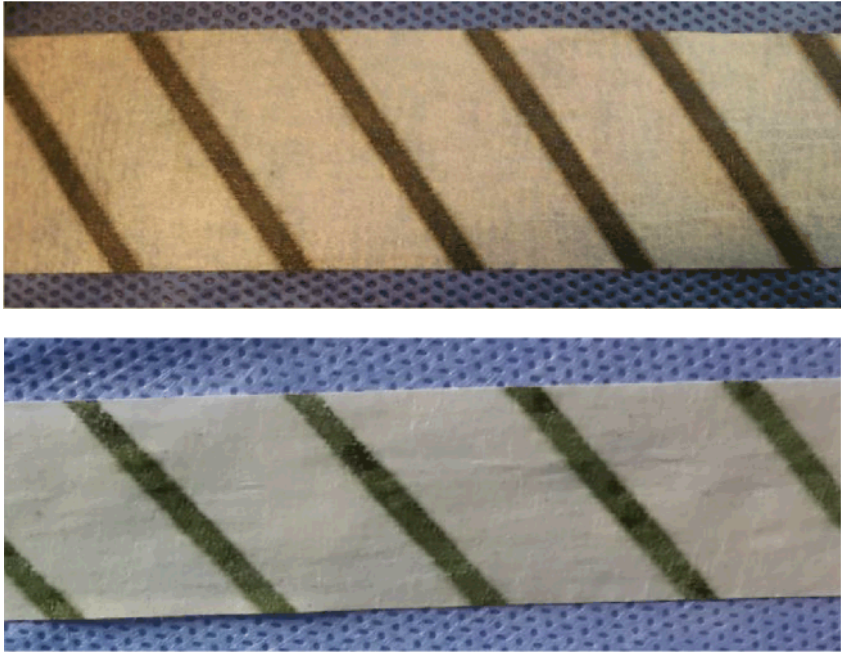
<b>Brand Name of Product</b>	STERIKING® Sterilization Tapes																				
<b>Generic Name of Product</b>	Sterilization Tapes																				
<b>Product Code Number(s)</b>	ITS19GL, ITS25GL, TPEDS-1, TPEDS-2, TPEDS-3																				
<b>Purpose of Product</b>	STERIKING® Sterilization Tapes are manufactured for closing packaged items that require wrapping for sterilization in hospitals and other similar uses.																				
<b>Range of Applications for Product</b>	Instrument wraps and other items that need to be taped closed during sterilization.																				
<b>Key Specifications of Product</b>	<p>STERIKING® sterilization tapes with indicator are produced by using strong impregnated crepe paper coated with an adhesive. This is principally based on natural, dry rubber and tackifying synthetic resins.</p> <table border="1"> <thead> <tr> <th><u>Property</u></th> <th><u>Units</u></th> <th><u>Typical Value</u></th> </tr> </thead> <tbody> <tr> <td>Thickness</td> <td>μ</td> <td>140–170</td> </tr> <tr> <td>Adhesion to Steel</td> <td>N/25 mm</td> <td>9.0–10.0</td> </tr> <tr> <td>Tensile Strength</td> <td>N/25 mm</td> <td>70–90</td> </tr> <tr> <td>Elongation</td> <td>%</td> <td>7</td> </tr> <tr> <td>Color</td> <td>Natural, indicator tape printed with colored stripes</td> <td>N/A</td> </tr> </tbody> </table>			<u>Property</u>	<u>Units</u>	<u>Typical Value</u>	Thickness	μ	140–170	Adhesion to Steel	N/25 mm	9.0–10.0	Tensile Strength	N/25 mm	70–90	Elongation	%	7	Color	Natural, indicator tape printed with colored stripes	N/A
<u>Property</u>	<u>Units</u>	<u>Typical Value</u>																			
Thickness	μ	140–170																			
Adhesion to Steel	N/25 mm	9.0–10.0																			
Tensile Strength	N/25 mm	70–90																			
Elongation	%	7																			
Color	Natural, indicator tape printed with colored stripes	N/A																			

### Shipping & Storage

<b>Shipping Conditions &amp; Requirements</b>	N/A
<b>Storage Conditions</b>	It is recommended that the STERIKING® products are kept in the original, closed transport cartons and stored in dry and clean conditions—protected from direct sunlight, excessive moisture, and heat.
<b>Packaging Contents</b>	<p>STERIKING® sterilization tapes are packed in recyclable, brown, hard carton cases. As an inner cover against moist and dust, the steam indicator tapes are wrapped in a recyclable high-density polyethylene (HDPE) sheet.</p> <p><i>Labeling:</i> Each case bears a label with the necessary information/instructions of the content in accordance with ISO 11140-1:2005.</p>
<b>Shelf Life</b>	<p>(When stored according to instructions), STERIKING® Sterilization Tapes' shelf life is:</p> <ul style="list-style-type: none"> <li>• Two (2) years from opening</li> <li>• Four (4) years maximum from date of manufacture.</li> </ul>

### Instructions for Using Product

<b>Description of Use(s)</b>	Manufactured for closing packages of items requiring wrapped sterilization in hospitals and other similar uses.
<b>Preparation for Use</b>	Place new roll of tape in the dispenser.
<b>Diagrams (drawings, pictures)</b>	<p><b>Starting color of unexposed indicator of ITSG-tape:</b></p>

	<p><b>End colors of correctly exposed indicator of ITSG-tape: Fully exposed Brown/Black</b></p>  <p><b>Please note:</b> The STERIKING® ITSG indicator tapes' color change may vary due to differences in processing parameters. The indicators should not be exposed to direct light prior to use.</p>
<b>Steps for Use of Product</b>	<ul style="list-style-type: none"> <li>• Use tape to close packages and items for sterilization.</li> <li>• Indicator (Type 1) tapes with steam indicator change color from white to brown/black.</li> </ul>
<b>Interpretation of Results</b>	N/A
<b>Contraindications of Test Results</b>	N/A
<b>Documentation</b>	N/A
<b>Special Warnings and Cautions</b>	<ul style="list-style-type: none"> <li>• Adhesive contains dry, natural rubber, which is processed from dry, natural rubber latex. <ul style="list-style-type: none"> <li>○ Conversion dramatically reduces the latex protein content in the final tape product.</li> <li>○ The presence of minimal quantities (0.2–0.4%) of latex protein could cause symptoms in people with a strong latex allergy.</li> </ul> </li> <li>• Skin contact with these adhesives is incidental and short term.</li> <li>• Do not expose sterilization tapes to direct light prior to use.</li> </ul>
<b>Disposal</b>	N/A

<b>Reprocessing Instructions</b>	
<b>Point of Use</b>	N/A
<b>Preparation for Decontamination</b>	N/A
<b>Disassembly Instructions</b>	N/A
<b>Cleaning – Manual</b>	N/A
<b>Cleaning – Automated</b>	N/A
<b>Disinfection</b>	N/A
<b>Drying</b>	N/A
<b>Maintenance, Inspection, and Testing</b>	N/A
<b>Reassembly Instructions</b>	N/A
<b>Packaging</b>	N/A
<b>Sterilization</b>	<p><b>Steam</b></p> <p>The steam indicator ink will react positively when subjected to heat and moisture in the steam autoclave. After sterilization, strong, dark lines appear on the backing of the tape. The usual time and temperature combinations are:</p> <ul style="list-style-type: none"> <li>• Three (3) minutes at 134 °C (273.2 °F)</li> <li>• Fifteen (15) minutes at 121 °C (249.8 °F).</li> </ul>
<b>Storage</b>	N/A

<b>Additional Information</b>	N/A
<b>Related Healthmark Products</b>	N/A
<b>Other Product Support Documents</b>	Sterilization Price List, Sterilization Brochure
<b>Reference Documents</b>	STERIKING® Sterilization indicator tapes conform to the international standard: ISO 11140-1 2005 (Type 1, process indicators)
<b>Customer Service Contact</b>	Healthmark, A Getinge Company 18600 Malyn Blvd. Fraser, MI 48026 1-586-774-7600 <a href="mailto:healthmark@hmark.com">healthmark@hmark.com</a> <a href="http://hmark.com">hmark.com</a>